


Optimized VHH Selection Affinity and Titer before Purification



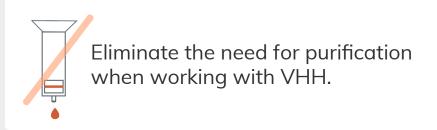




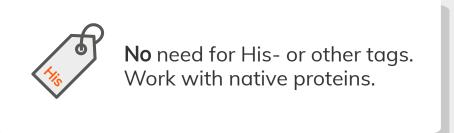


Fidabio Clone Selection

Single point size-ranking of VHH clones


The Fida 1 size measurement is resulting from expression levels and affinity combined.

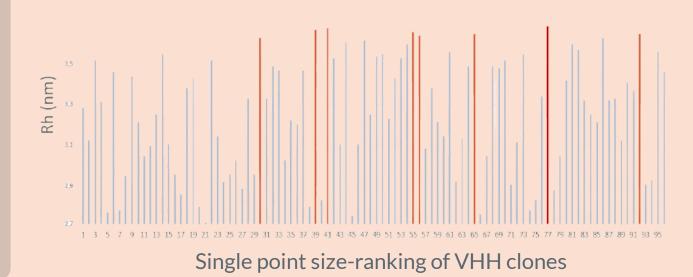

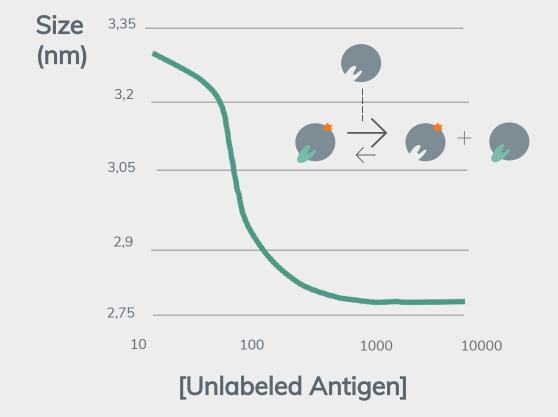

Competitive assay on selected clones Titrating unlabelled antigen into a mixture of unpurified VHH solution and labelled antigen decreases size until the minimum value where all the labeled antigen is free. Size is linked to the fraction of VHH bound, therefore, the affinity and the expression level of VHH are assessed simultaneously.

Detailed characterization of best VHH clone(s) Clone(s) with the best combination of affinity and expression level are produced in larger scale, purified and further characterized.

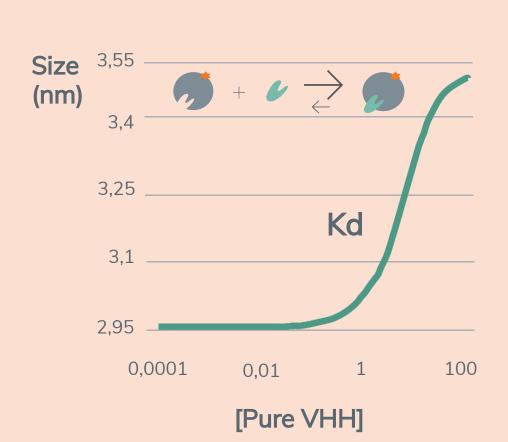

Fida Biosystems ApS Generatorvej 6 2860 Søborg Tel.: +45 53 72 78 70

